
RingCommunications

Scanner to Control Room Intercom System – Pulse

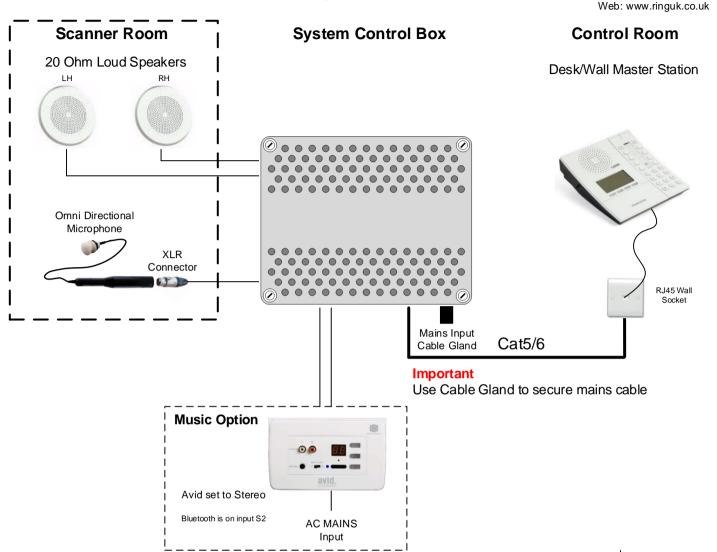

Ring Communications (UK) Ltd

Newmarket Business Centre

Newmarket, Suffolk, CB8 0AT Tel: +44(0) 1638 660 629

E-Mail sales@ringuk.com

341 Exning Road

Installation

Desk/wall station should be mounted with easy access to controls. System Control Box can be mounted in the control room with access for maintenance. Cable between Desk/wall Station and the System Control Box is CAT5 cable. Cable for microphone should be microphone cable, 2 core plus Screen. The speaker requires 2 core speaker cable, use same type cable between Avid if fitted. See Avid installation guide.

Recommendations

Microphone must be fitted where it can pickup speech and not equipment noise. Keep away from aircon units. Loudspeakers and Microphone must be spaced so that there is no Feedback, <u>More than one metre apart.</u>

Operation

To communicate with the patient on the Scanner, press the Star key"*", then press and hold the "M" key to talk to the patient, let go to return to listen mode.

Patient in the theatre, cannot hear operator without the "M" key being pressed. When Pressing the "M" key, relay will cut music from Avid.

Avid Settings

Bluetooth setup codes are under face plate, Bluetooth input is on input S2 See Avid Manual for operational instructions.

Close System

To cancel all communications (Switch OFF) press Cancel. Music will still be heard from Avid to speakers. Press ON/OFF button on Avid to turn OFF, then switch off music source.